

# Superior Accuracy Performance of FreeStyle Libre 3 Sensor in a Head-to-Head Study Against Dexcom G7




The first head-to-head study comparing the FreeStyle Libre 3 system and Dexcom G7 system.<sup>1</sup>



Multicenter, single-arm, prospective study to assess point accuracy of FreeStyle Libre 3 system and Dexcom G7 system head-to-head



Data was obtained from 55 adult subjects enrolled with T1D or T2D treated with insulin. Subjects wore both sensors simultaneously




Accuracy assessed by comparing CGM sensor data with venous blood glucose levels\* and capillary blood glucose values†

## STUDY CONCLUSION‡

“ The FreeStyle Libre 3 sensor was **more accurate** than the Dexcom G7 sensor in all metrics evaluated throughout the study period. ”

### HEAD-TO-HEAD COMPARISON OF FREESTYLE LIBRE 3 AND DEXCOM G7 SYSTEMS (VENOUS BLOOD GLUCOSE REFERENCE)

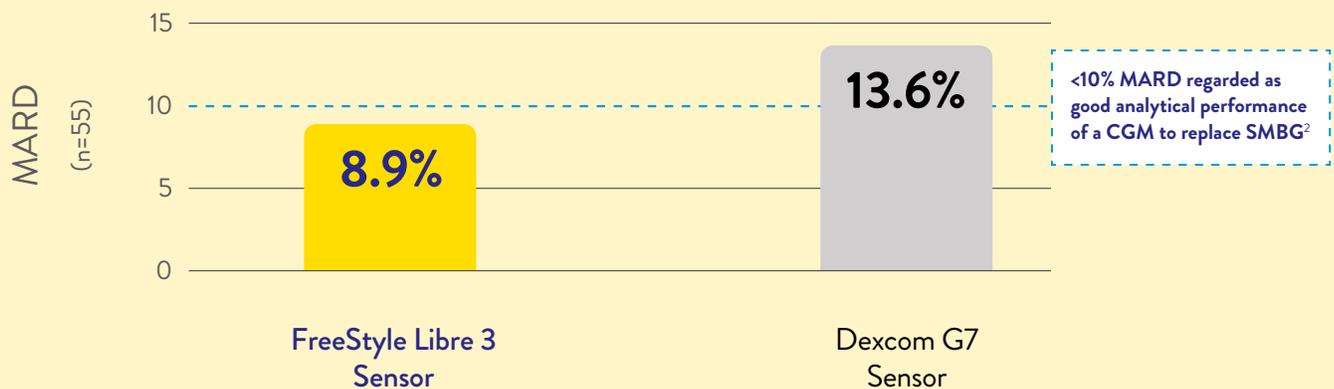


CGM = continuous glucose monitoring; MARD = mean absolute relative difference; SMBG = self-monitoring blood glucose; T1D = type 1 diabetes; T2D = type 2 diabetes.

\*Measured using the Yellow Springs Instrument as the laboratory reference in 3 in-clinic sessions of 8 hours.

†Measured using the FreeStyle Libre 14 Day Flash Glucose Monitoring System Reader with FreeStyle Neo test strips at least 8 times per day.

‡Based on a multicenter, nonsignificant risk, head-to-head study comparing FreeStyle Libre 3 and Dexcom G7 sensor data in identical conditions. Outcome measures: differences in mean absolute relative difference, differences in overall percentage  $\pm 20$  mg/dL/ $\pm 20$ . Results from 55 subjects (42 minimum sample size required). Study sponsored by Abbott.

# FreeStyle Libre 3 Sensor Significantly Outperforms Dexcom G7 in a Head-to-Head Accuracy Study

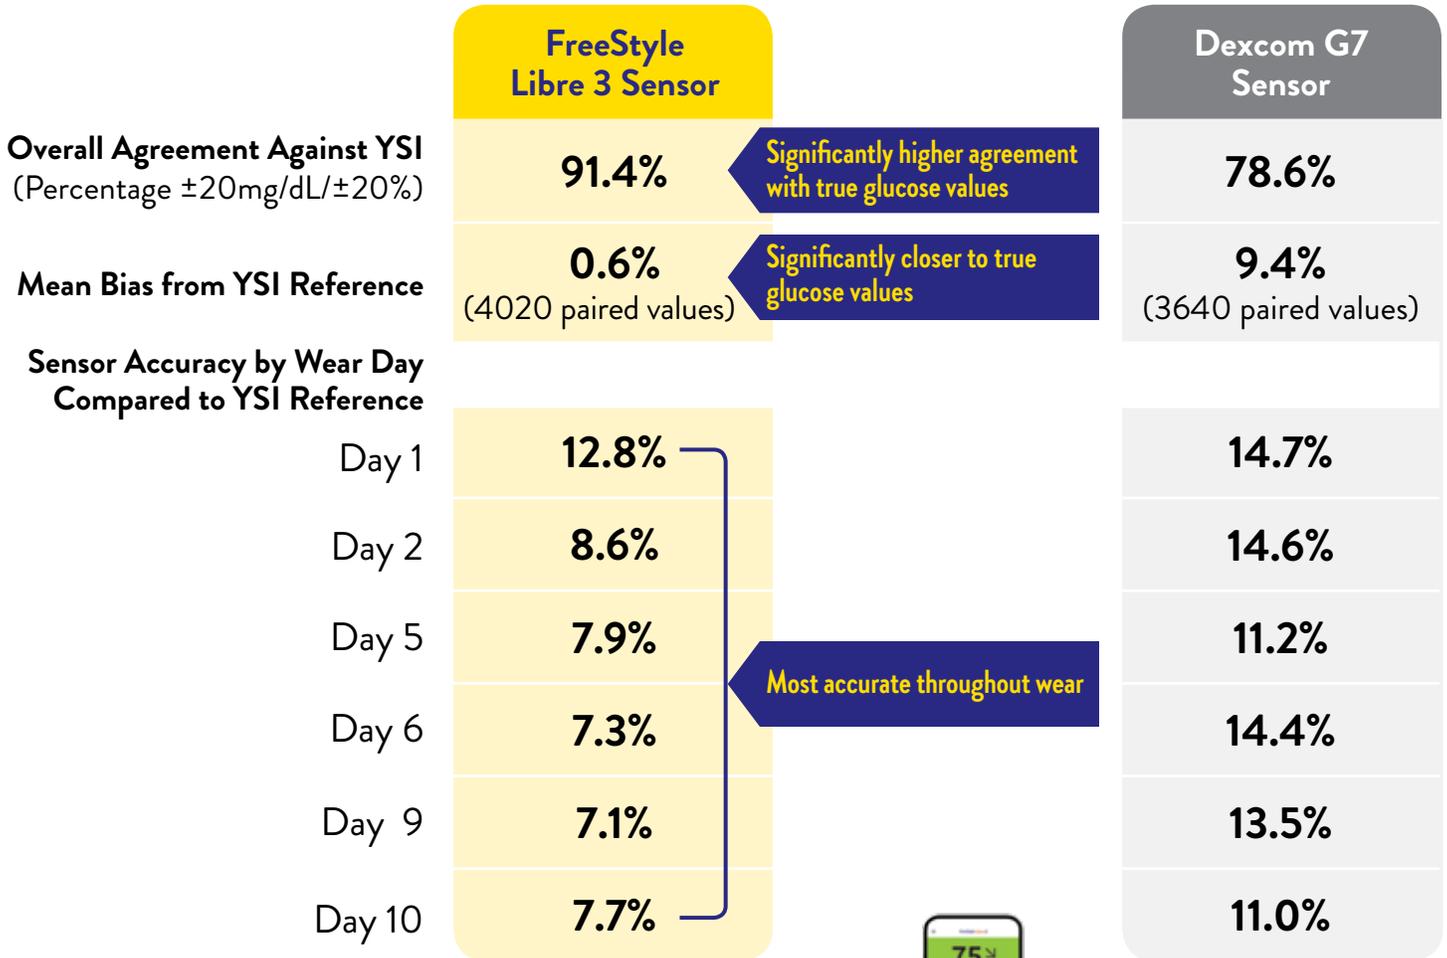

**Superior Accuracy Performance of FreeStyle Libre 3 sensor:**  
Most accurate in a head-to-head study vs Dexcom G7.<sup>1</sup>




1. Hanson K, et al. Comparison of point accuracy between two widely used continuous glucose monitoring systems. *J Diabetes Sci Technol.* 2024;1-10. doi: 10.1177/19322968231225676  
 2. Kovatchev BP, et al. Assessing sensor accuracy for non-adjunct use of continuous glucose monitoring. *Diabetes Technol Ther.* 2015;17(3):177-86. doi: 10.1089/dia.2014.0272  
 The sensor housing, FreeStyle Libre, and related brand marks are marks of Abbott. Other marks are the property of their respective owners. FreeStyle Libre 3 is a medical device CE 2797. Material intended only for healthcare professionals. Not for public distribution or public display. © 2024 Abbott. ADC-88195 v1.0 02/2024